

An evaluation of sit to stand devices for use in rehabilitation

M. Fray PhD, S. Hignett PhD, A. Reece, S. Ali, L. Ingram
Loughborough Design School, Loughborough University, UK

1. Introduction

When a patient requires an assistive device to help with the activity of raising from a seat there are many devices that can deliver the support and movement needed. The functional movement for transport, patient movement or hygiene requirements is common place in care settings. The design and action of most sit to stand assistive devices is considered to be active as the device requires some balance, trunk control and weightbearing ability in the person being assisted. There is concern that the movement is mostly passive and the support and structure of the device creates and controls all movements in the lower limbs due to fixation at the trunk and knee.

Modern acute healthcare has a clear focus reducing the length of stay in any setting. Consequently any advantage that can be gained by encouraging rehabilitation and a faster improvement in ability is welcomed. For a normal unassisted sit to stand there is a known sequence of actions which are not entirely matched in the assisted actions. This study explores the patterns of movement in natural movement against the movements seen in assisted transfers.

In this study the Sara® Flex was shown to:

- Allow more forward knee movement during raising and lowering
- Allowed more bodyweight through the feet during raising
- Give one of the closest Centre of Pressure movement patterns to the natural active movement
- The Sara Flex was the most preferred device in this trial.
- The Sara Flex encourages the participant to be more active through sitting and standing assisted transfers

2. Objectives:

To explore the relationships between the movement patterns in an unassisted active sit to stand, and active stand to sit, and the movements recorded when using sit to stand assistive devices for both tasks. This study compares joint movement, body weight through the feet and the centre of pressure through the feet across a number

of devices. Subjective evaluations of all devices were also completed to evaluate the user comparison of the devices.

3. Methods:

The trial followed a fully squared repeated measures design where all participants (n=20) were exposed to all conditions (n=7, unassisted active plus 6 devices). The order of presentation was balanced to give appropriate comparison. Participants were required to complete 3 sit to stands and 3 stand to sits with each device. All data collection methods were piloted with a small number of participants before committing to the full trial.

3.1 Participants:

Participants were acquired from local recruitment. All were required to be 55+ years, no restrictions were placed on medical history but each had to be able to complete the sit to stand action independently. For all transfers the participants were requested to raise/lower themselves to the highest/lowest position possible with the device.

3.2 Subjective Data Collection:

After each set of transfers with any device (n=3 repetitions) a range of subjective evaluations were requested from the participant inquiring:

- Comfort during and after transfer
- Security during and after transfer
- Sling fitting
- Quality of the knee support
- Overall performance

All subjective evaluations were recorded on 5 point likert scales (5 being preferred score). After all devices were completed a post study interview was conducted. The experimenter recorded verbal comments and the participant was asked to rate their preference or dislike for various aspects of the devices.

- Overall preference of device
- Preferred slings
- Preferred knee support

3.3 Physical Data Collection

The movements completed were recorded with 3 methods; video recordings were taken as a record of each transfer, the ground reaction force was recorded using a 6 dimensional force plate, the limb positions and limb angles were recorded with motion capture (Codamotion with Odin Software).

The data used for analysis was:

- Force measured through force plate
 - Vertical co-ordinate
- Centre of Pressure location (anterior to posterior, AP)
- Joint positions from motion capture
 - Foot - Toe, 5th Metatarsal and Heel
 - Fibula – Lateral Malleolus and Fibula Head
 - Femur - Epicondyle and Greater Trochanter
 - Pelvis – Anterior and Posterior Iliac Spine
 - Shoulder - Acromion
- Joint Angles
 - 3D Euler angle calculations were performed by the ODIN software for ankle, knee, hip
- Video recordings were used for clarification.

3.4 Conditions:

The study compared an unassisted action with the device assisted transfers. The active movement was self-selected, participants could use hands to assist but this was not included in the analysis. 5 comparison devices were purchased (B-F) from the marketplace and adapted to allow for the data collection described above. Device G was a prototype device which had an innovative flexible silicone knee support (Sara Flex). All devices were used in accordance with the manufacturers instructions for operation and sling

fitting. The sling fitting, set up and controls were controlled by the experimenter.

The conditions were:

- A. Active motion no assistance (Control)
- B. Knee/shin support, lever lift, sling, flat footplate
- C. Knee/shin support, lever lift adjustable, sling, flat footplate
- D. Knee support, Straight line lift, sling, flat footplate
- E. Knee support, lever lift, sling, flat footplate
- F. Knee/shin support, lever lift, sling, angled footplate
- G. Silicone knee support, lever lift, sling, flat footplate


4. Results

Participant characteristics (n = 20) were all over 55 years, mass 44.4-109.9 kgs, height 147.3-187.9 cm. Medical histories were recorded but none were excluded.

The physical data was filtered for missing data and erroneous data which was all removed. The movement was identified as starting at when the hip marker was raised/lowered 20 mm and finished when the hip marker ceased movement. This gave comparable time frames with only the movement phases being included. To allow comparison between transfers many data were normalised to percentage figures e.g. time, weight, centre of pressure across the foot length etc.

4.1 Subjective Results


The subjective scores were recorded on 5 point Likert scales. Judgements for raising and lowering were combined. 5 being the positive score and 1 being the least regarded.

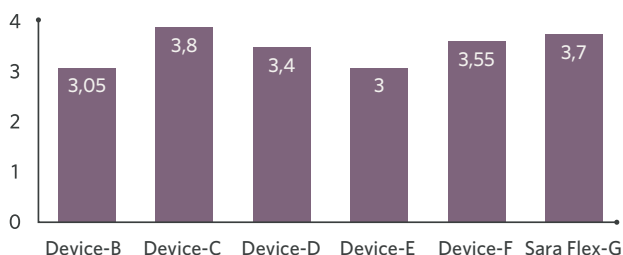

Graph 1.

Average comfort during the movement


showed that for comfort the Sara® Flex and Device C were the most comfortable.

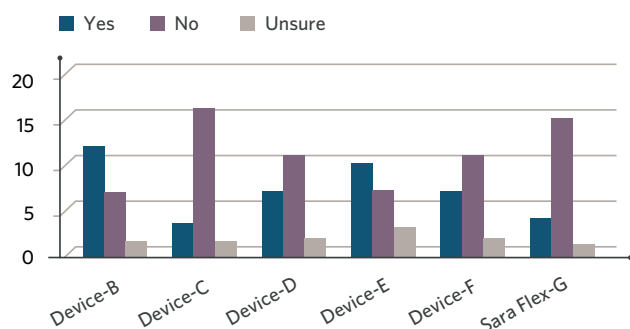

Graph 2.


Participants reporting sling movement

The sling movement had a clear relationship with the sensations of comfort and security. Graph 2 showed the frequency that reported the sling moving. Devices B, E, D and F reported the most movement with C and the Sara® Flex being the least movement.

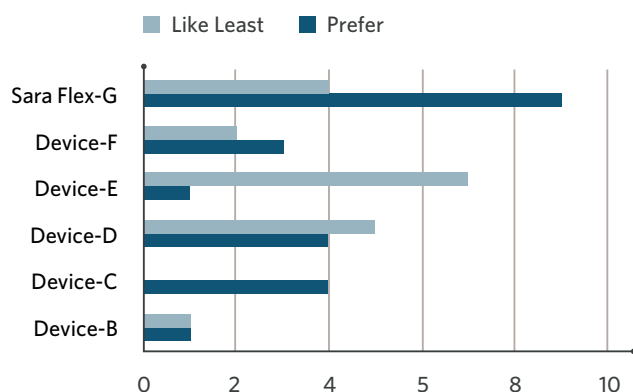


Graph 3.
Preference and dislike ratings for devices overall

After the participant had used all devices for all repetitions the post-trial interview revealed a preference for the Sara® Flex device. Participants reported the most preferred and the least preferred across the devices. Graph 3 indicates the most preferred votes for the Sara® Flex however it should be noted that individual feedback recorded that some thought the flexibility felt less secure than others in the range.

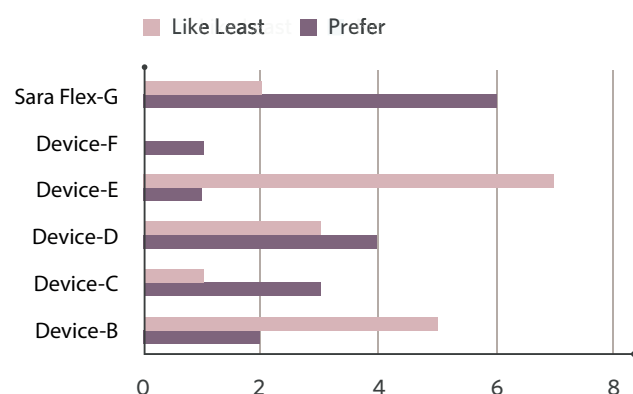

Graph 4.
Preference and dislike ratings for slings

Graph 4 shows the ratings for the sling preference. Devices B and E recorded more negative views than positive. Specifically E had a slow and very vertical lift pattern which increased the slippage of the sling against the participant. The devices D, C and G had more positive than negative ratings. The Sara® Flex device showed the most positive response. Interestingly F and G had identical slings but the combination with the silicone knee support affected the ratings.

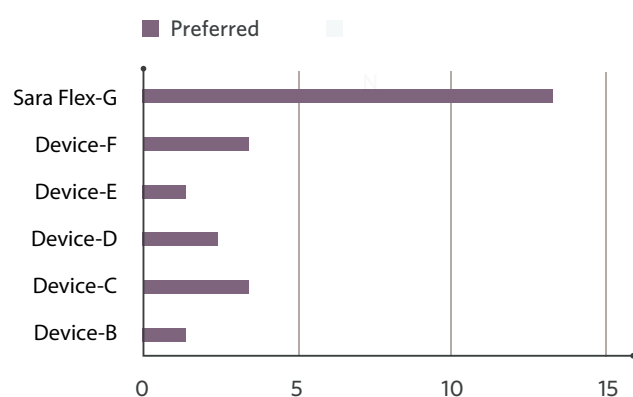

Graph 5.
Preference for knee supports

Whilst some participants considered the silicone knee support to lack security Graph 5 show the overwhelming preference for the Sara® Flex knee support during the trial.

Graphs 3, 4 & 5 show Sara® Flex to be the most preferred device.

4.2 Subjective Summary


There was a high level of comfort and security with device C and the Sara® Flex devices. Both devices were more appreciated by the participants. Specifically the innovative silicone flexible knee support was the most positive factor in the comfort review. The comparison with natural movement was not possible with the group as they lacked an insight into rehabilitation requirements.

4.3 Physical Results

The first results were used to understand the movement components of the active sit to stand. There was good variation between participants with good correlation between the repetitions for each participant.


Graph 6. Active Sit to Stand - Centre of Pressure and % Bodyweight

Graph 6 shows the % bodyweight (%BW) and the position of the centre of pressure (CoP). The CoP plot shows how the weight starts approx. 60% towards the heel and as the person stands the weight moves forward towards the toe and then back again once in standing. The %BW is characterised by a rapid onset of force as the weight comes off the seat and there is maximum acceleration up to standing.

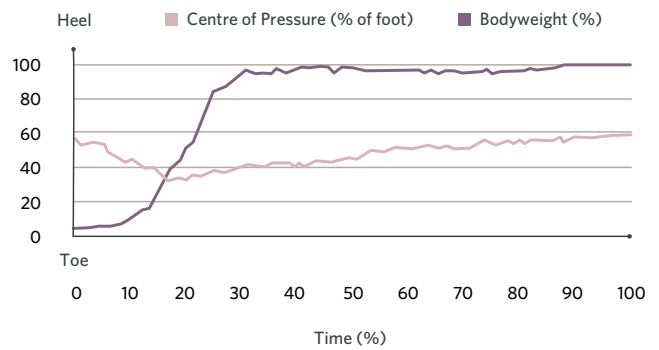


The main aim of this study was to explore the relationship between the movement pattern in the active tasks and those reported in the assisted transfers. The analysis of the movement for the active sit to stand showed forward movement of the knee with forward lean of the trunk to allow the weight to

be taken on the feet to allow vertical acceleration into standing and a corresponding extension at hip, knee and ankle. The following graphs show some movement comparisons between the devices and the active sit to stand.

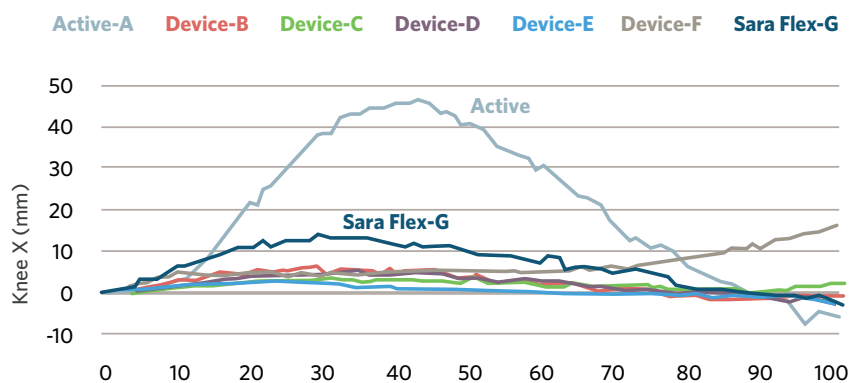

Graph 7. Forward Knee Movement

Graph 7 shows the horizontal movement of the knee as it comes forward over the toes in standing. The closest device to the active curve is the Sara® Flex which is significantly higher movement than all other devices ($P < 0.05$).

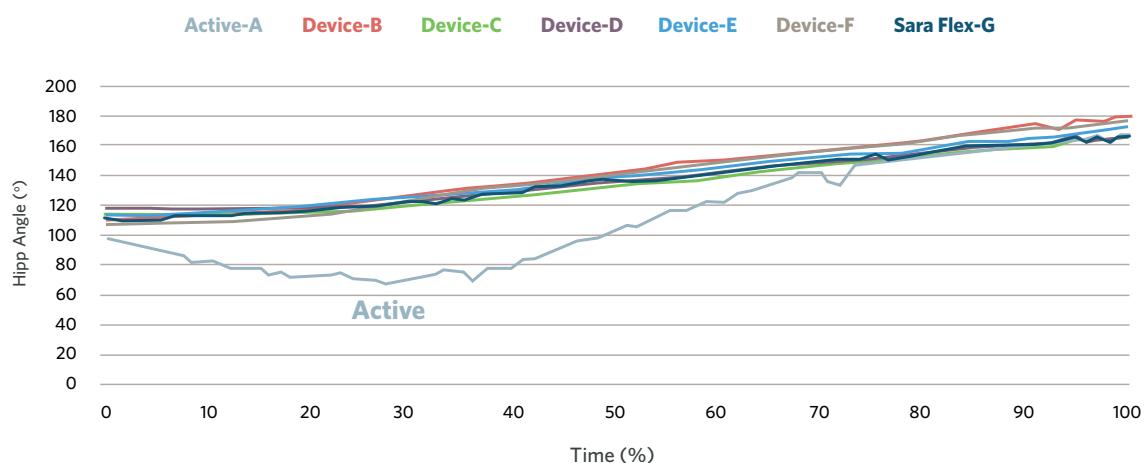


Graph 8. Hip Angle During Sit to Stand

Graph 8 shows the angle between the trunk and the thigh. As the person moves forward the angle closes and the curve of the median hip angle drops below the assisted movement curves. The backward lean into the sling allows

only the steady increase from 90° to upright approximately 180° for all devices. Similar comparisons were seen in the angles of knee and ankle where movement was seen in the active but much less in the device assisted.



Graph 9.
% Bodyweight for the Sit to Stand Action

The clearest benefit of the flexible knee support was the effect on the ground reaction force. The Sara® Flex allowed up to 70% of the body weight to be measured at the standing position which was significantly higher than most other devices ($p < 0.05$).

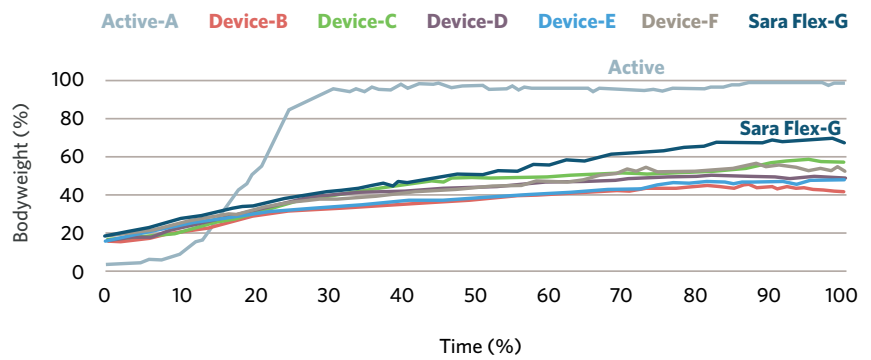

Graph 10.
% Centre of Pressure for Sit to Stand

The experimental team expected the CoP for the devices to be much further to the heel as the centre of gravity and centre of mass is supported by the device outside the base of support. The results show that the CoP movement is much closer to the active pattern than expected. This is explained by the response to being pulled forward by the sling. The participant braced themselves against the footplate and hence the CoP moved forward towards the toe.

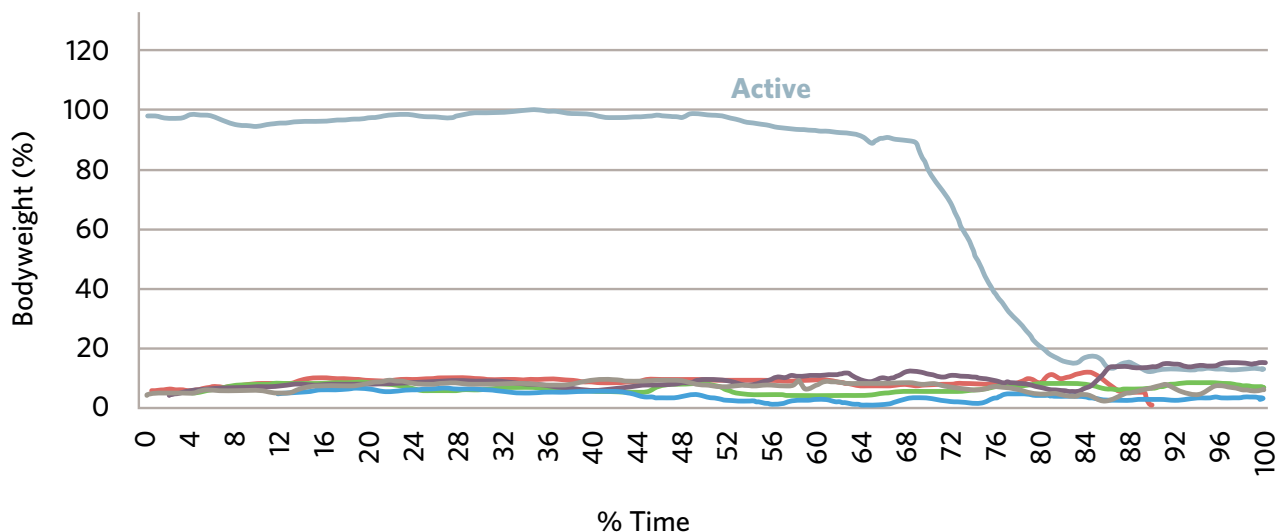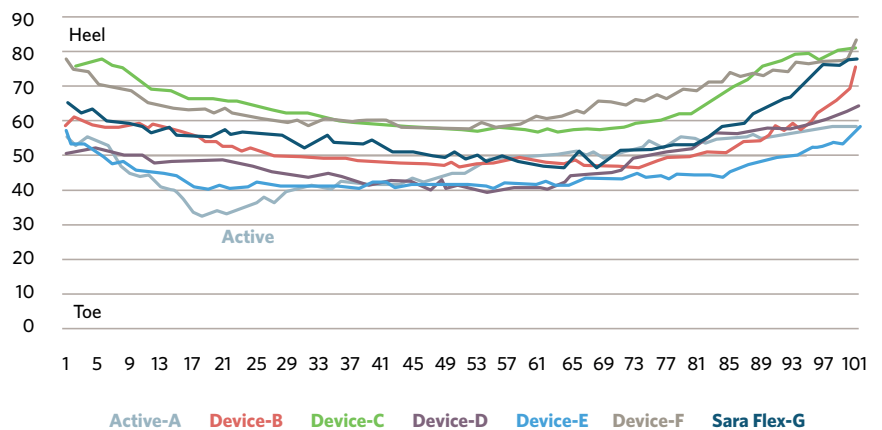

Graph 11.
% Bodyweight for Stand to Sit

In the data that was collected for the stand to sit actions the patterns of movement for horizontal knee movement, hip, knee and ankle angles were all very similar and did not follow the active movement pattern. There was however a significant change in the bodyweight data. Graph 11 shows that the force being registered at the force plate for the sitting action was very small for all assisted sitting actions. The Sara® Flex had

the highest % bodyweight but was still a small percentage. This dramatic reduction in ground reaction force is a key finding. The video analysis showed that the participants lowered themselves into the knee support and took tension in the sling as per the instruction. This created a physical support between the two fixed positions and made the knee the primary weight bearing structure and not the feet.

4.4 Physical Summary.

The Sara® Flex showed some positive differences to the other devices in this trial and in several data sets was closest to the active pattern of movement.

This investigation reported:

- When assisted people push into the floor and CoP moved towards the toe
- When over lifted CoP moved towards the toe as weight decreases
- Sara Flex allowed more forward movement at the knee
- Sara Flex allowed more weight through feet compared to other devices
- Sara Flex showed quicker transfer of weight onto feet like 'normal' stand
- During lowering (stand to sit) very low bodyweight was recorded from all devices.

5. Concluding Remarks

The distribution of the bodyweight in the different movements is an interesting finding when considering the question of using the devices as an aid to rehabilitation.

The Sara® Flex allowed more forward knee movement, allowed more bodyweight through the feet and gave one of the closest CoP movement patterns to the active unassisted transfer. With these differences the Sara® Flex was still the most preferred device in this trial. These component actions show that the Sara® Flex encourages the participant to be more active through sitting and standing assisted transfers.

Specifically, it should be noted that for an unassisted active stand to sit transfer stronger eccentric muscle activation is required to support lowering. Adding a level of voluntary control in the persons own muscles to support their descent would raise the activity level for people who are assisted. This increase in activity will improve their route to improved function and rehabilitation goals. In our modern healthcare systems this may support an earlier access to rehabilitation and lead to an earlier recovery.

PH.CF.02.1.GB-INT.1.AHG - Sara flex White paper. Jan 2018. Only Arjo designed parts, which are designed specifically for the purpose, should be used on the equipment and products supplied by Arjo. As our policy is one of continuous development we reserve the right to modify designs and specifications without prior notice.

At Arjo, we are committed to improving the everyday lives of people affected by reduced mobility and age-related health challenges. With products and solutions that ensure ergonomic patient handling, personal hygiene, disinfection, diagnostics, and the effective prevention of pressure ulcers and venous thromboembolism, we help professionals across care environments to continually raise the standard of safe and dignified care. Everything we do, we do with people in mind.

Arjo AB • Hans Michelsensgatan 10 • 211 20 Malmö • Sweden • +46 10 335 4500

www.arjo.com

